



PRODUCT
PROTECTION



VERTICAL LAMINAR FLOW CABINET LORICA

The cabinet is designed for protection of agents and materials inside the cabinet working chamber from external and cross-contamination in the ductless pure air environment.

The cabinet is used for work with substances which are not hazardous for the personnel health.

The cabinet is used to equip individual working places in medical, pharmaceutical and other institutions working with high requirements for air purity in the working zone.





LAMSYSYSTEMS

Vertical Laminar Flow Cabinet

LORICA

BAVnp-01-Laminar-S.

APPLICATION

- Quality control in pharmaceutical and food industry;
- Ophthalmological solution preparation;
- Culture media preparation;
- Optical mechanics manufacture;
- Electronics industry;
- Pharmaceutical industry.

DISTINCTIVE FEATURES

The microprocessor system SintelL-1 controlling the fan motor allows to minimize the power consumption of the cabinet, to reduce the level of acoustic and electromagnetic noise.

The system of air consumption static regulation AIS LS automatically regulates air balance in the working chamber by changing the number of fan revolutions according to the level of filters contamination. Upon reaching the threshold value of contamination the system activates the warning alarm.



1200 mm 1500 mm 1800 mm



**PRODUCT
PROTECTION**


- The illumination block is taken out of the working chamber and does not initiate air flow turbulence.
- Coloring of the cabinet is made with the powder enamel resistant to disinfectant solutions.
- The control unit with LCD indicates the switching of the systems, their possible malfunctions, the operation mode chosen and the technological timer.
- HEPA filter is held by springs providing filter leak tightness for the whole lifetime.
- The electronic shield panel provides easy operation and disinfection.

PERFORMANCE CHARACTERISTICS OF THE CABINET LORICA

Air cleanliness class in the working chamber of the cabinet for suspended particles content – according to GMP – according to ISO 14644-1	A 5 ISO
Class of supply HEPA filter in accordance with the EN 1822-1	H14
Class of prefilter in accordance with the EN 779	G4
Airflow pattern characteristics in the working chamber of the cabinet	downflow unidirectional (laminar)
Average downflow velocity in the working chamber: – factory specified velocity, m/s – recommended range of velocity for independent adjustment whereby the uniformity of air flow is maintained, m/s	0,40 0,25 – 0,50
Illuminance level in the working zone, Lux, not less than	1000
Noise level at 1m distance from the cabinet (at the centerline of the working opening, with the front window sash in the working position), dB, not more than	55



PARAMETERS AND DIMENSIONS OF THE CABINET LORICA

BAVnp-01-Laminar-S	1200	1500	1800
Article	1E-D.001-12.0	1E-D.001-15.0	1E-D.001-18.0
Dimensions of the cabinet assembled with the stand /WxDxH/, mm	1200x760x1870	1500x760x1870	1800x760x1870
Dimensions of the working zone /WxD/, mm	1130x625x650	1430x625x650	1730x625x650
Mass of the cabinet assembled with the stand, kg, not more than	160	186	206
Maximum input power of the cabinet excluding the load on the built-in outlet unit, W, not more than	410	410	590
Accepted load on the built-in outlet unit, W, not more than	1000	1000	1000

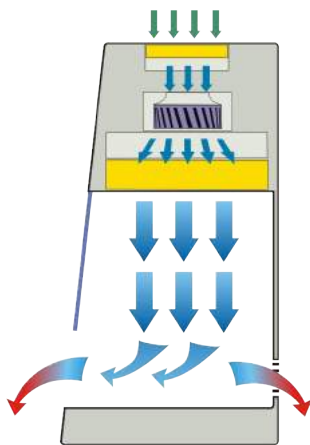

AIR FLOW SCHEME


- contaminated air
- room air
- clean (filtered) air

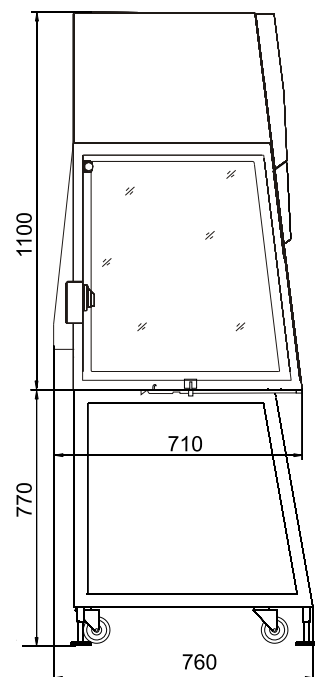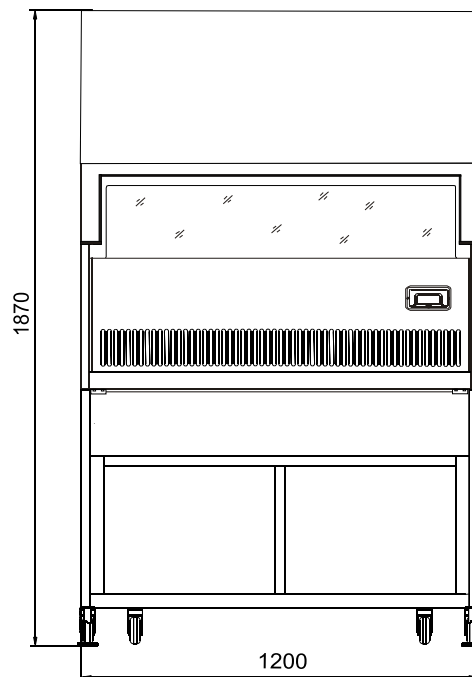

VERTICAL LAMINAR FLOW CABINET

LORICA

PRODUCT PROTECTION

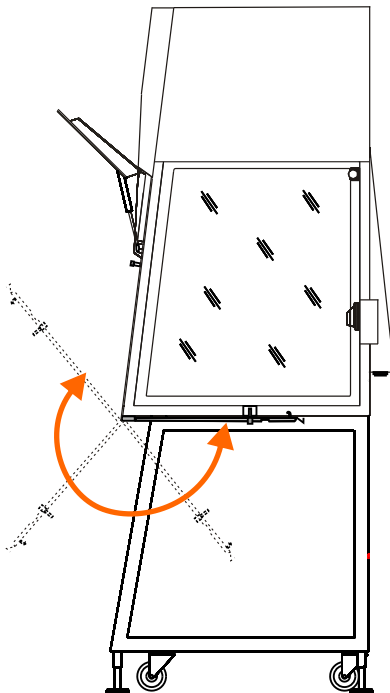

The protection plate is designed to prevent direct exposure of operator to UV irradiation during the disinfection of the working chamber.

Also the protection plate is recommended for placement when the cabinet is not used for a long time.

Tel.: +49 (0) 30 9489 2080
Fax.: +49 (0) 30 9489 2081
info@lamsys-euro.com

www.lamsys.com

**LAMSYS GmbH**

Campus Berlin-Buch
Robert-Rössle-Str. 10
D 79 (Erwin-Negelein-Haus)
13125 Berlin
Deutschland/Germany

Published in 2018

Manufacturer reserves the right to change technical specifications and construction design in the process of further technical improvement of equipment.